


Sample Name: konak

```

=====
Acq. Operator   :
Acq. Instrument : Instrument 1                Location : Vial 101
Injection Date  : 14.06.2022 13:13:21      Inj      : 1
                                           Inj Volume : 1 µl

Acq. Method     : D:\CHEM32\1\METHODS\VODKA_2019.M
Last changed    : 08.06.2022 14:22:28
Analysis Method  : C:\CHEM32\1\DATA\2022-06-14 SIS\SIG1G1001752.D\RUN.M
Last changed    : 20.06.2022 13:18:05
                 (modified after loading)
Method Info     : 25.06.2019 H2
=====

```

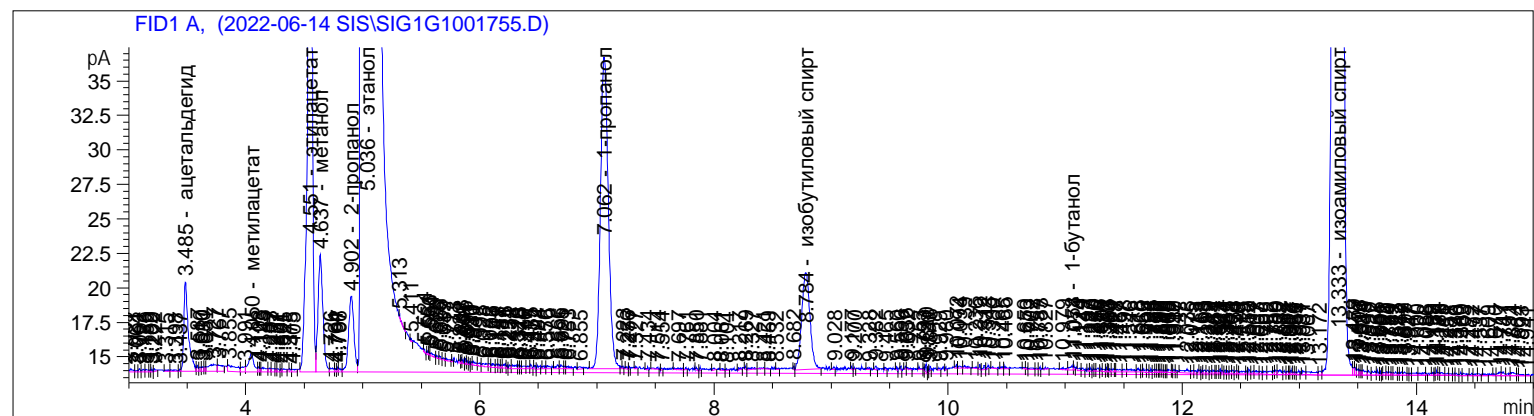

```

=====
Internal Standard Report
=====

```

```

Sorted By           :      Signal
Calib. Data Modified :      20 June 2022 г. 13:18:05
Multiplier:         :      1.0000
Dilution:           :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Sample ISTD Information:

ISTD #	ISTD Amount мг/л безво	Name
1	7.89270e5	этанол

Signal 1: FID1 A,

RetTime [min]	Type	ISTD used	Area [pA*s]	Amt/Area ratio	Amount мг/л безво	Grp	Name
3.485	VV	1	17.58351	1.56500	100.46136		ацетальдегид
4.050	VV	1	4.13836	1.76261	26.62953		метилацетат
4.551	BV	1	129.27979	9.93171e-1	468.74197		этилацетат
4.637	VV	1	24.71154	1.41378e-4	1.27544e-2		метанол
4.902	VV	1	17.55067	9.40935e-1	60.28821		2-пропанол
5.036	VBAS I	1	2.16195e5	1.00000	7.89270e5		этанол
7.062	VV T	1	104.47670	7.03202e-1	268.21247		1-пропанол
8.784	VV T	1	34.64483	6.29313e-1	79.59476		изобутиловый спирт
11.058	VV T	1	5.61411e-1	6.20938e-1	1.27265		1-бутанол
13.333	PV T	1	854.89056	5.98564e-1	1868.10131		изоамиловый спирт

Sample Name: konak

Totals without ISTD(s) : 2873.31500

1 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

=====

*** End of Report ***